



IF IN DOUBT ASK

THIRD ANGLE PROJECTION



DO NOT SCALE

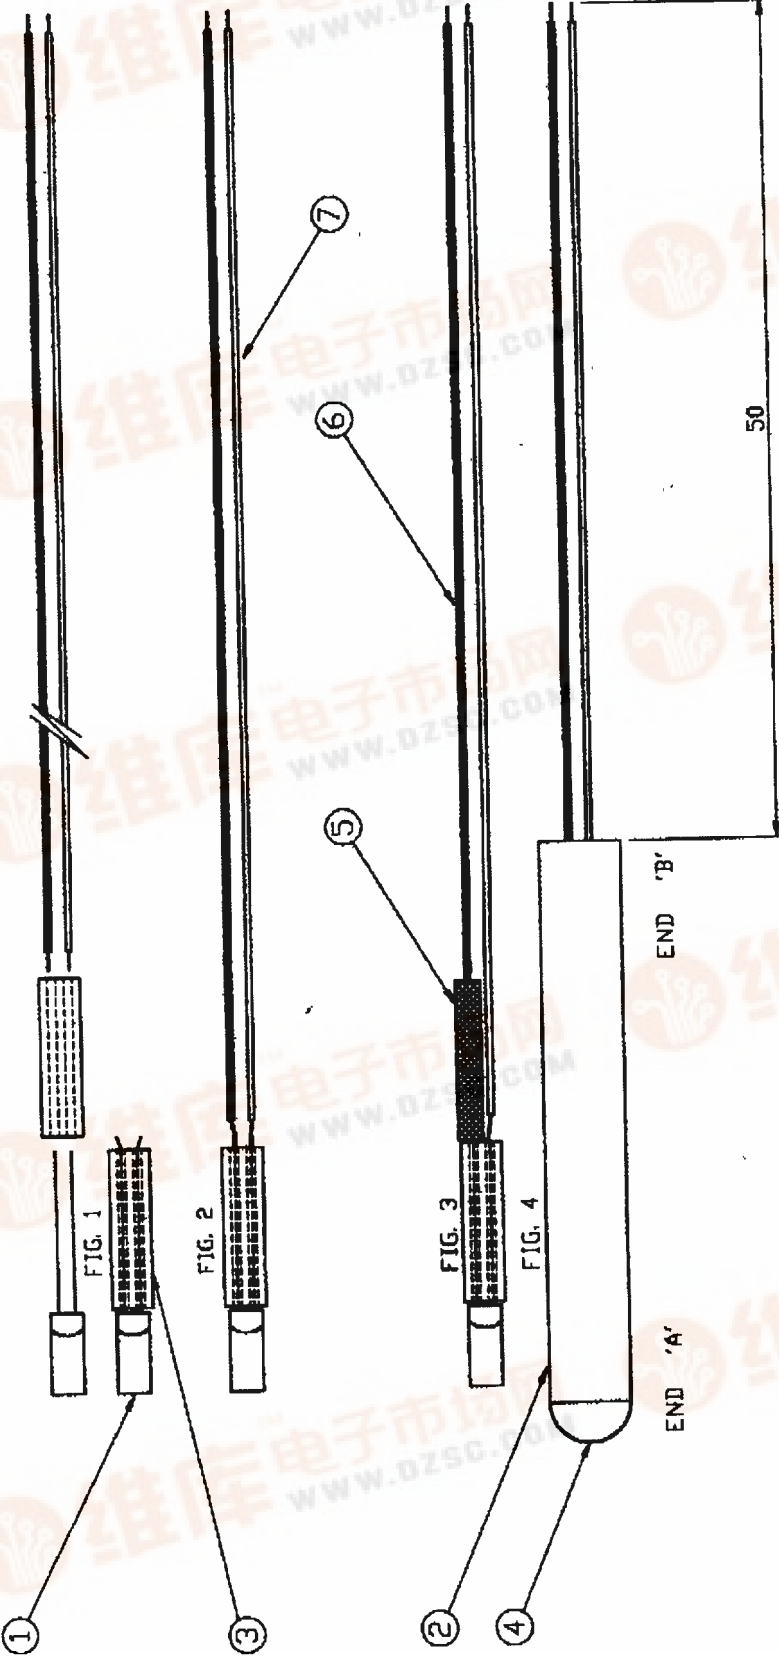

**CONTROLLED**

- NOTES:
- 1, CUT ITEM 6 TO 100mm, AND TRIM INSULATION BACK.
  - 2, REPEAT FOR ITEM 7.
  - 3, SLIDE ITEM 3 ONTO ITEM 1 (FIG. 2).
  - 4, SPOT WELD OR MICROWELD ITEM 6 & ITEM 7 ONTO ITEM 1 (FIG. 3).
  - 5, SPLIT ITEM 5 OVER JOIN BETWEEN ITEM 6 & ITEM 1 AND SHRINK IN POSITION.
  - 6, SLIDE ITEM 5 OVER JOIN BETWEEN ITEM 6 & ITEM 1 AND SHRINK IN POSITION.
  - 7, INSERT ASSY. INTO ITEM 2 SO ITEM 5 IS SUB FLUSH WITH THE END OF ITEM 2.
  - 8, MIX ITEM 8 INTO STIFF PASTE AND APPLY INSIDE END 'A' ENSURING THAT ITEM 1 IS FULLY ENCAPSULATED. FORM END INTO DOME AND ALLOW TO HARDEN.
  - 9, CHECK ASSY. FOR CONTINUITY & RESISTANCE.
  - 10, INSERT ITEM 8 (RUNNY CONSISTENCY) INTO END 'B' AND CURE, 1 HOUR IN OVEN @120°C OR 24 HRS @ ROOM TEMP.
  - 11, REPEAT NOTE 9.
  - 12, CUT WIRES TO REQUIRED LENGTH.

DRAWING No. 010011MF		DRAWN: J.S.C.		CHECKED:		DATE: 23.11.98		SCALE: N.T.S.	
TITLE: CERAMIC PRT. ELEMENT B		DRAWING No. 010011MF		PART NUMBER: RSE237-1657		FARNELL: 725-5731		SHEET 2 OF 3 SHEETS	
TOLERANCE: +0.25 UNLESS STATED OTHERWISE		TOLERANCE: -0.25 DOES NOT APPLY TO ASSY. DWGS		LAB FACILITY LIMITED, 99 WALDEGRAVE ROAD, TEDDINGTON, MIDDLESEX, TW11 8LR		TEL: 0181 9435331		FAX: 0181 9434351	
MATERIAL: SEE NOTES		FINISH: SEE NOTES		DATE: 23.11.98		DRAWN: J.S.C.		APP: [ ]	
ISSUE: A		REFER TO NDR 009		REASON FOR CHANGE: [ ]		DATE: [ ]		DRAWN: [ ]	
THIS DRAWING REMAINS THE PROPERTY OF LAB FACILITY LIMITED AND MAY NOT BE REPRODUCED WITHOUT OUR PERMISSION									

