

A compact low-cost LED module ideally suited for applications where a bright display under all conditions is required. The DPM 40 is fitted with high efficiency LEDs and supplied with a filter and bezel to give a high contrast display. The small size and low cost of the unit makes it

- 🕒 11mm (0.43") Digit Height
- 🕒 Programmable Decimal Points
- 🕒 Auto-zero
- 🕒 Auto-polarity
- 🕒 200mV d.c. Full Scale Reading (F.S.R.)
- 🕒 Display Hold



SCALING


Two resistors Ra and Rb may be fitted in order to alter the full scale reading (F.S.R.) of the meter - see table. The meter will need re-calibration.

Required F.S.R.		Ra	Rb
2V	Note	910k	100k
20V	Note	1M	10k
200V	Note	1M	1k
2kV	Note	1M	100R
200µA		LINK	1k
2mA		LINK	100R
20mA		LINK	10R

NOTE
Ensure that link across Ra is OPEN.

Specification	Min.	Typ.	Max.	Unit	Stock Number
Accuracy (overall error) *		0.05	0.1	% (±1 count)	
Linearity			±1	count	
Sample rate		3		samples/sec	
Operating temperature range	0		50	°C	
Temperature stability		150		ppm/°C	
Supply voltage	4.5	5	5.5	V	
Supply current		100	200	mA	
Input leakage current (Vin = 0V)		110		µA	

* To ensure maximum accuracy, re-calibrate periodically.

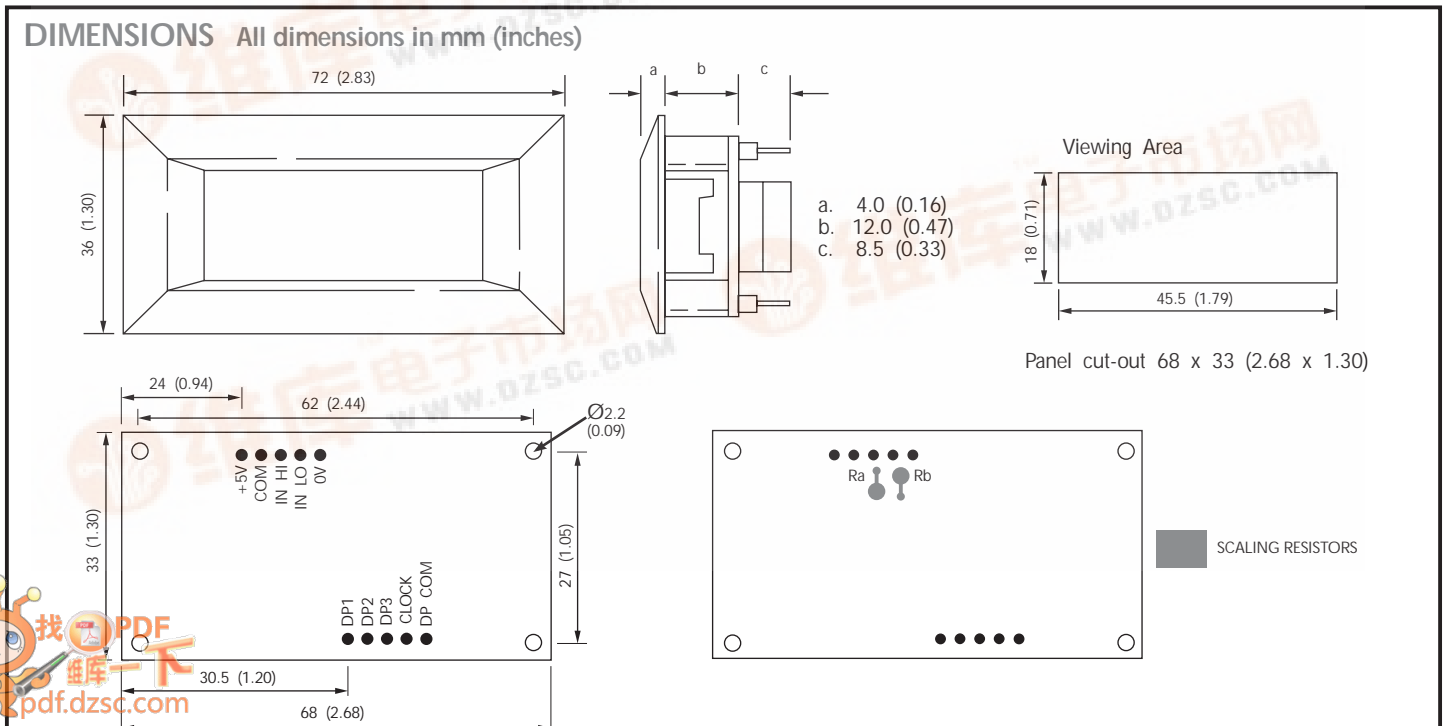


PIN FUNCTIONS

- A. DP1 199.9
 - B. DP2 19.99
 - C. DP3 1.999
 - D. CLOCK/ HOLD Connect to 0V to hold display reading. Leave open for normal operation.
 - E. DP COM Connect to Pin A, B or C to select required DP.
 - 1. +5V Positive power supply input.
 - 2. COM The ground for the analogue section of the converter, held actively at 2.8V (nom) below +5V. This pin is for use only when the module is used with a fully floating supply. **It should on no account be connected to any other terminations or circuitry except as specified in the relevant operating modes.**
 - 3. IN HI Positive measuring input.
 - 4. IN LO Negative measuring input.
 - 5. 0V Negative power supply input.
- } Analogue inputs must be no closer than 1V to the positive supply or lower than 1.5V below 0V.



SAFETY

To comply with the Low Voltage Directive (LVD 93/68/EEC), input voltages to the module's pins must not exceed 60Vdc. If voltages to the measuring inputs do exceed 60Vdc, then fit scaling resistors externally to the module. The user must ensure that the incorporation of the DPM into the user's equipment conforms to the relevant sections of BS EN 61010 (Safety Requirements for Electrical Equipment for Measuring, Control and Laboratory Use).

VARIOUS OPERATING MODES



Operation with input referenced to panel



Operation with input floating with respect to power supply.